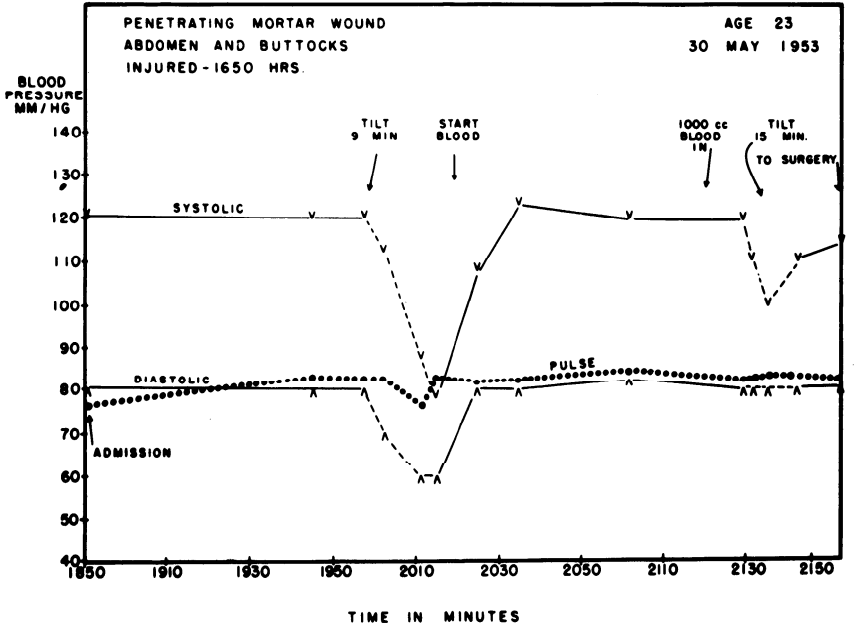Evaluation of Use of a Standard Tilt Test